

1040-1

Off-Line Airborne Effluent Monitor

The 1040-1 Off-Line Airborne Effluent Monitor assures radioactive materials within airborne effluents do not exceed maximum permissible concentrations (MPC) by alarming when safe levels are exceeded, protecting personnel from possible exposure to excessive radiation.

The Code of Federal Regulations requires any effluent that could possibly contain radioactivity be monitored, and the 1040-1 Off-Line Airborne Effluent Monitor meets the guidelines set forth in the United States Nuclear Regulatory Commission (USNRC) radiation protection standards. Off-line gas monitors are frequently used in conjunction with particulate monitors. This is particularly the case with a stack or duct where effluent is released into the environment. Used in this manner, the particulate monitor serves as a pre-filter for the gaseous monitor and also as a monitor for airborne radioactive particulates. Where an off-line gas monitor is used independently, without the aid of a particulate monitor, a separate filter assembly is installed to prevent contaminated particulate buildup inside the sensitive volume. The off-line effluent monitor incorporates its own pumping system to ensure a positive displacement of the effluents being monitored. Off-line effluent monitoring is normally utilized where optimum geometry is desired to gain maximum sensitivity. Scintillation detectors are used because of their sensitivity and reliability.



Key features

- Universal Digital Ratemeter with dynamic range up to 107 CPM.
- Scintillation type detectors.
- Optimized sampling geometry for maximum sensitivity
- Rugged open frame skid construction for ease of maintenance.
- Positive displacement type pumping system.
- Automatic pressure compensation for gas density.
- Class 1E qualification available.
- Off-line airborne effluent monitoring skid.
- Measures and reports airborne radioactive releases from stacks and ducts.
- Quantifies airborne particulate, radioiodine and gaseous effluents.
- Compatible with the 953 Series Detectors and the 1042 Series Digital Ratemeters.



Trusted
radiation
monitoring.

The sample is drawn from the process stack/duct via isokinetic nozzles (when required), through customer's sample line to the inlet of the sampling skid. The sample passes through the particulate and iodine filters, then through the gas sample volume to the pumping system and back to the process stack/duct. The sample flow is controlled by a manual set point, or ratioed to stack/duct flow for isokinetic requirements. The detector output signal is transmitted to the Universal Digital Ratemeter. The particulate ratemeter displays gross particulate counts, the iodine ratemeter displays iodine counts as determined by the preset window of the single channel analyzer, and the gas ratemeter displays gross noble gas counts, compensated for changes in pressure at the volume chamber. These ratemeters also provide output alarm contacts for Alert, High Radiation, Channel Fail, and when required Rate Of Rise for fixed filter application. A Low Flow alarm is also available for the sample stream. Check source actuation is manual from the ratemeter, with alarms muted when in the check source mode.

Sample inlet:

1 inch OD stainless steel tubing, compression fitting

Sample outlet:

0.75 inch OD stainless steel tubing, compression fitting

Maximum internal pressure:

10 psig

Dynamic count range:

10 to 10^7 CPM

Gas sample volume:

3000 cc (see other models below)

Skid weight:

3000 lb (1360.8 kg)

Particulate filter paper:

Hollingsworth & Voss #LB-5211-A-O with a collection efficiency of 99.97 % for particles 0.3 micron and larger

Iodine filter:

Charcoal cartridge

Compatible detectors:

953 Series Beta and Gamma Scintillation Detectors

Note: *Optional grab sampling capability available for particulate, iodine, noble gas and tritium.*

The off-line airborne effluent monitor consists of the following components:

Open-frame sampling skid, with the following components mounted, plumbed and wired:

- Gas sampler, fixed volume, with 4 pi lead shielding as required, 841-334
- Particulate/Iodine samplers, as required, with 4 pi lead shielding
- Scintillation type detectors, as required
- Pressure transmitter upstream of gas sampler for automatic compensation of count rate for gas density
- Mass flow controller for isokinetic sample flowrate control
- Positive displacement pumping system
- Valving and plumbing, as required
- Isokinetic gas nozzle assembly for the stack/duct (when required)
- Universal Digital Ratemeters, local or remote mounting

Technical specifications

Power requirements


120 V ac, 50/60 Hz, 1 phase

Sample flow rate

1 to 4 SCFM



Sample temperature limit

50 °F to 122 °F (10 °C to 50 °C)

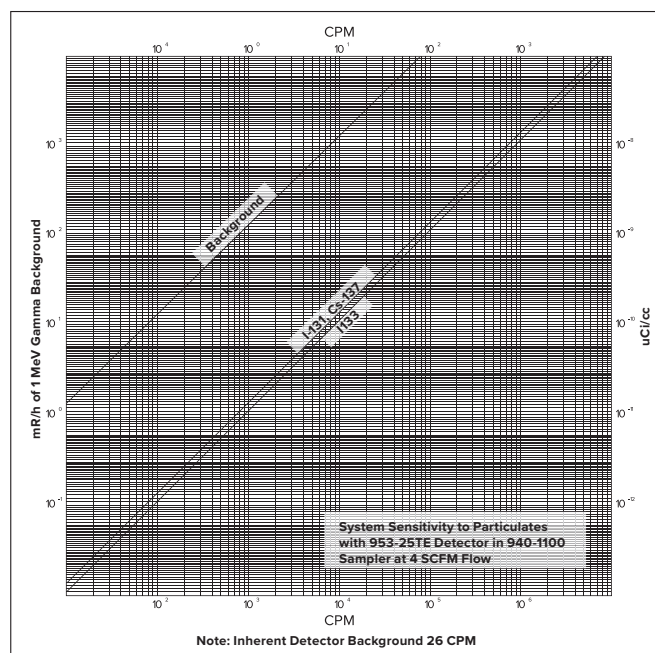



Trusted
radiation
monitoring.

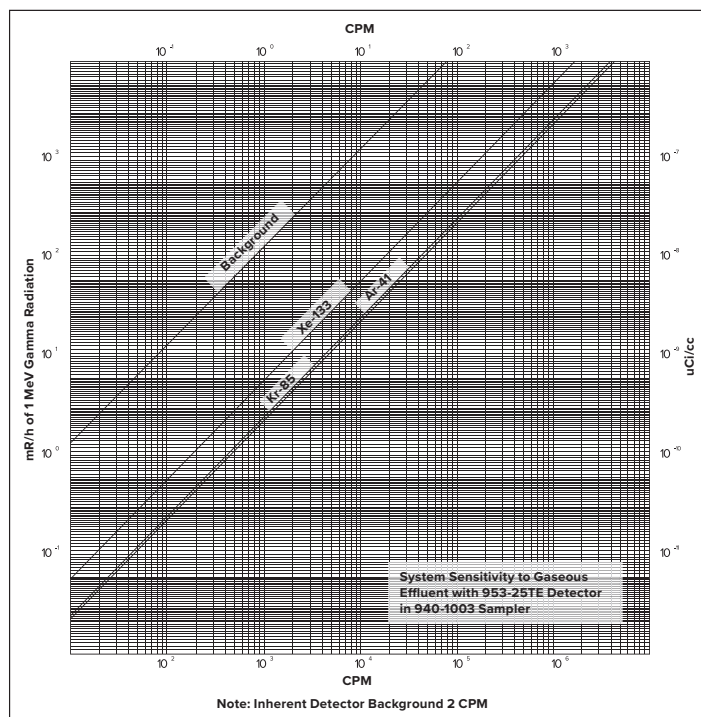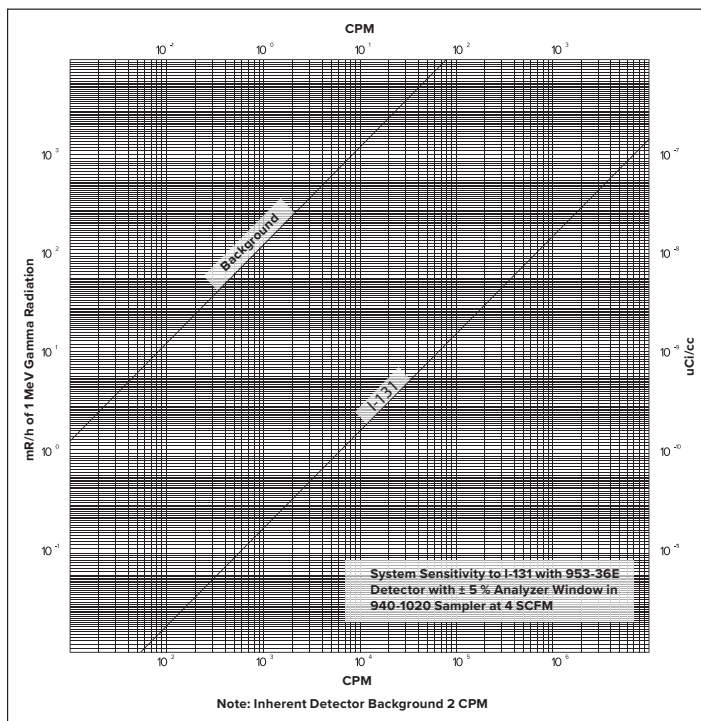

Ordering information

Model

1040-1-111, Normal Range Particulate, Iodine, and Noble Gas Monitoring System.

1040-1-101, Particulate and Noble Gas Monitoring System.

1040-1-211, Particulate, Iodine, and Noble Gas Monitoring System with Moving Particulate Filter

1040-1-200, Moving Particulate Filter Monitoring System.

1040-1-001, Noble Gas Monitoring System

Notes & Options:

Other model variations are available. Please contact Sales@Victoreen.com for more information.

1. 1E Qualification available.
2. Seismic qualification available.
3. Local and remote ratemeters available.
4. PLC process control available.
5. Flow control options available.
6. Manual sampling options available.

FLUKE®

Biomedical

Fluke Biomedical.

Trusted for the measurements that matter.

Fluke Biomedical
28775 Aurora Road
Cleveland, OH 44139-3303 U.S.A.

For more information, contact us at:
(844) 847-8139 or Fax (440) 349-2307
Email: sales@victoreen.com
Web access: www.victoreen.com

©2014 Fluke Biomedical. Specifications subject to change without notice. Printed in U.S.A. 10/2014 3015215B_EN

Modification of this document is not permitted without written permission from Fluke Corporation.

FLUKE®
Biomedical

RaySafe™

LANDAUER®